


# Certificate of Analysis

SD-SS3E-03 Lot # 061819ES

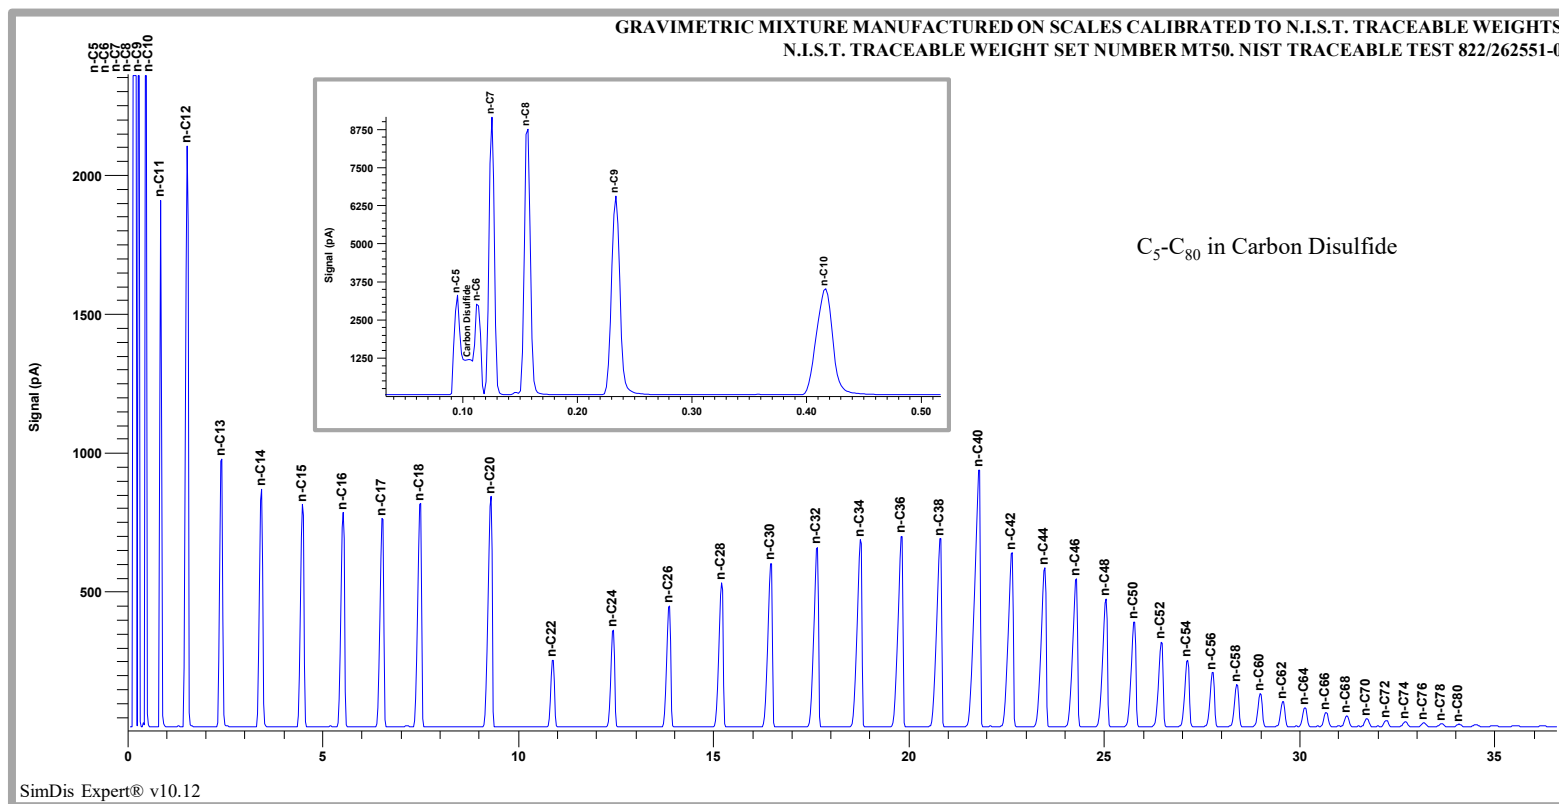

## SD-SS3E-03 Retention Time Standard for ASTM D7213

Lot #: 061819ES Exp: June 2024

Column: SD-002HTE2 (5m x 0.53mm x 0.1 $\mu$ m) Inlet: 80°C-380°C at 10°C/min Carrier: UHP He at 12 mL/min (constant flow)

Oven: 35°C-380°C at 10°C/min (10 min final hold) Detector: FID at 390°C Injection Volume: 0.2  $\mu$ L

 Separation Systems, Inc.  
Experts in Gas Chromatography

Phone 850-932-1433

Sales@SeparationSystems.com

www.SeparationSystems.com