


Certificate of Analysis

SD-SS3E-05 Lot # 080519ES

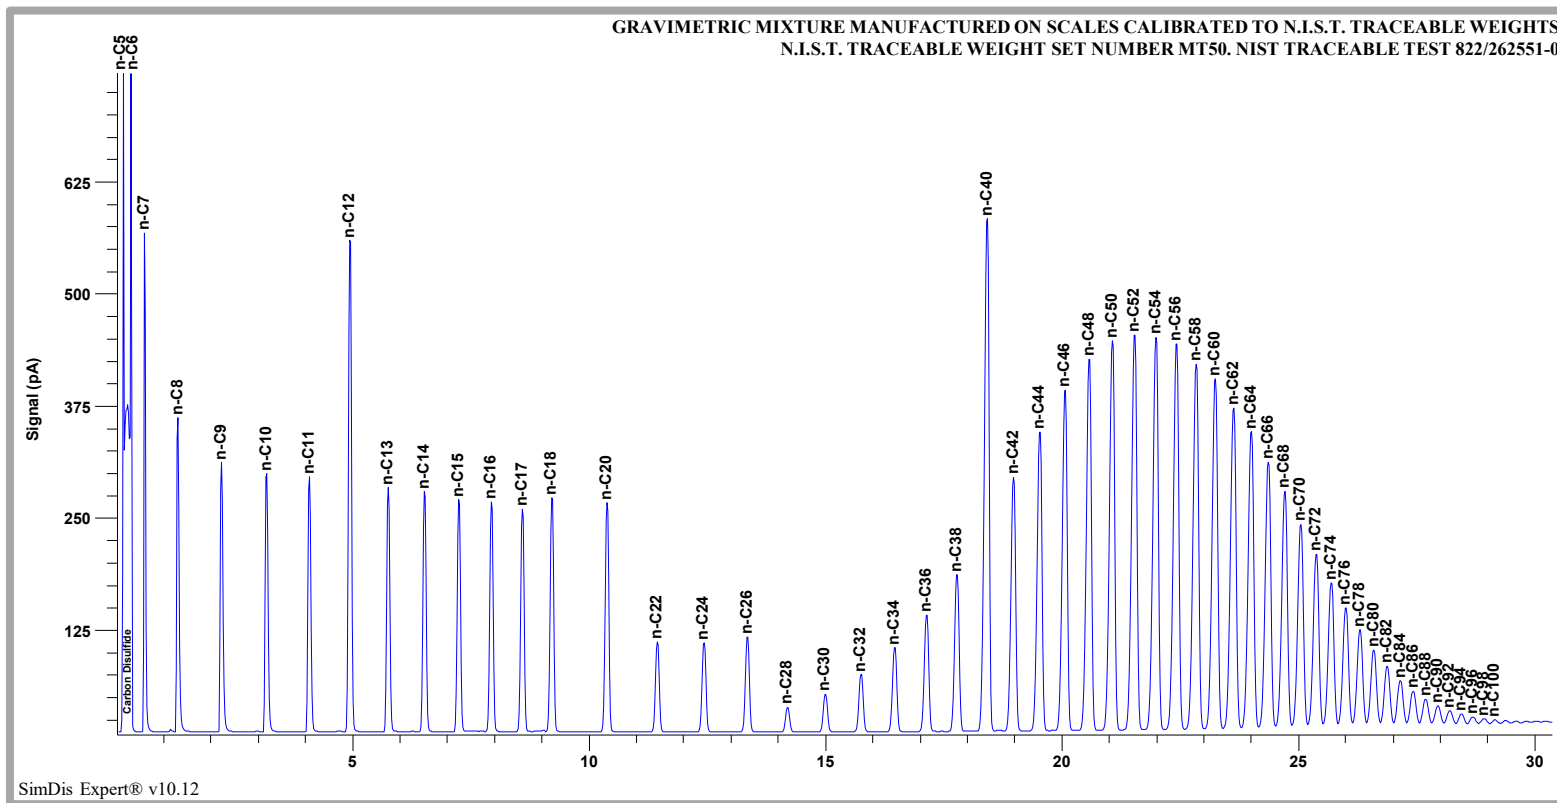

SD-SS3E-05 Retention Time Standard for ASTM D7169

Lot #: 080519ES Exp: Aug. 2024

Column: SD-002HTE2 (5m x 0.53mm x 0.1 μ m) Inlet: 35°C (0.5 min hold) to 425°C at 15°C/min Carrier: UHP He at 20 mL/min (constant flow)
Oven: -20°C (0.5 min hold) to 425°C at 15°C/min (5 min final hold) Detector: FID at 435°C Injection Volume: 0.2 μ L

 Separation Systems, Inc.
Experts in Gas Chromatography

Phone 850-932-1433

Sales@SeparationSystems.com

www.SeparationSystems.com