


Certificate of Analysis

SD-SS3E-02-WG Lot # 111716ES

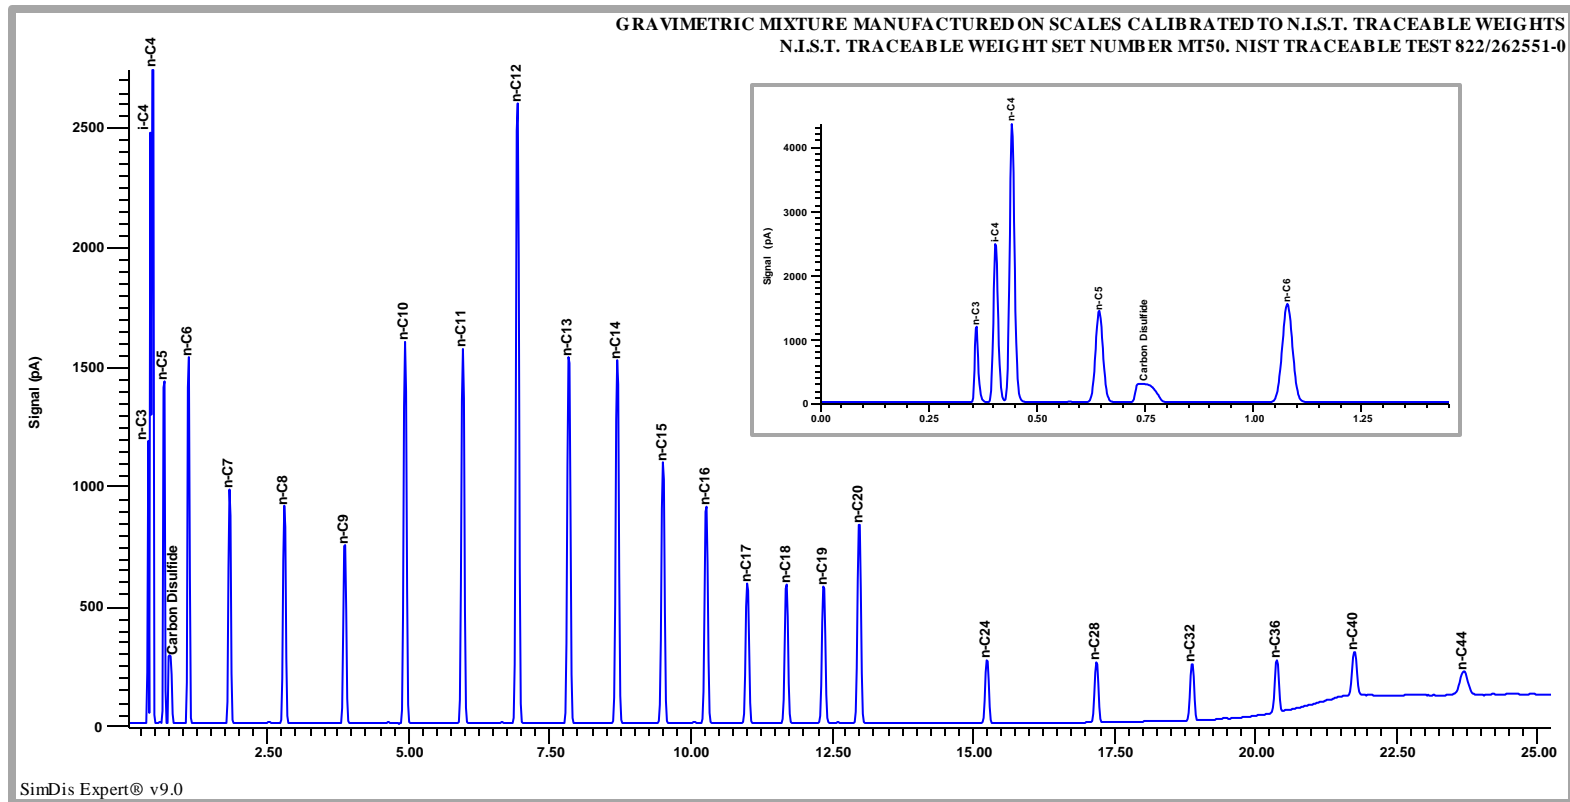

SD-SS3E-02-WG Retention Time Standard with Gases for ASTM D2887

Lot #: 111716ES Exp: Nov. 2021

Column: SD-002-2 (10m x 0.53mm x 2.65 μ m) Inlet: 80°C-350°C at 15°C/min Carrier: UHP He at 10 mL/min (constant flow)
Oven: 30°C-350°C at 15°C/min (10 min final hold) Detector: FID at 360°C Injection Volume: 0.2 μ L

 Separation Systems, Inc.
Experts in Gas Chromatography

Phone 850-932-1433

Sales@SeparationSystems.com

www.SeparationSystems.com