


Certificate of Analysis

SD-SS3E-03-WG Lot # 060717ES

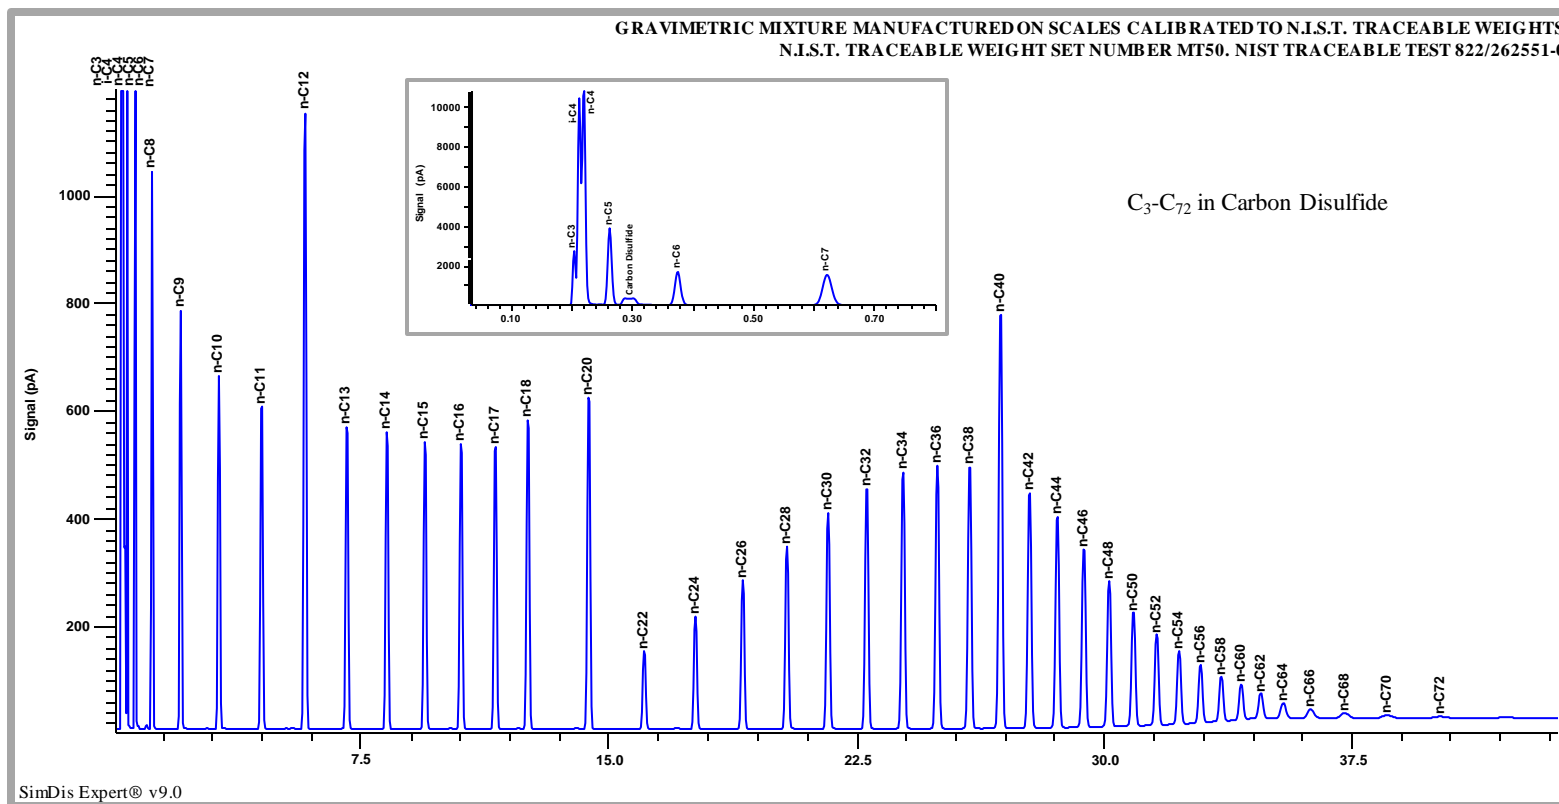

SD-SS3E-03-WG Retention Time Standard with Gases for ASTM D7213

Lot #: 060717ES Exp: June 2022

Column: SD-002-EX2 (10m x 0.53mm x 0.9 μ m) Inlet: 80°C-380°C at 10°C/min Carrier: UHP He at 12 mL/min (constant flow)
Oven: 35°C-380°C at 10°C/min (10 min final hold) Detector: FID at 390°C Injection Volume: 0.2 μ L

 Separation Systems, Inc.
Experts in Gas Chromatography

Phone 850-932-1433

Sales@SeparationSystems.com

www.SeparationSystems.com